

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA
 Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 0338
 CALIBRATION DATE: 07-Sep-12

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS

Soc = 0.2641
 Voffset = -0.7515
 Tau20 = 1.11

A = 8.2937e-003
 B = 3.7348e-005
 C = -6.4043e-006
 E nominal = 0.036

NOMINAL DYNAMIC COEFFICIENTS

D1 = 1.92634e-4 H1 = -3.30000e-2
 D2 = -4.64803e-2 H2 = 5.00000e+3
 H3 = 1.45000e+3


BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.24	6.00	0.05	1.217	1.12	-0.11
1.24	2.00	0.05	1.198	1.16	-0.08
1.25	12.00	0.04	1.276	1.14	-0.11
1.26	20.00	0.04	1.378	1.19	-0.07
1.26	26.00	0.04	1.467	1.21	-0.05
1.27	30.00	0.05	1.598	1.31	0.04
4.21	2.00	0.05	2.450	4.41	0.20
4.22	12.00	0.05	2.739	4.33	0.11
4.22	6.00	0.05	2.595	4.45	0.23
4.23	20.00	0.04	3.027	4.32	0.09
4.24	26.00	0.05	3.314	4.33	0.10
4.24	30.00	0.05	3.757	4.66	0.42
6.79	20.00	0.04	4.262	6.66	-0.13
6.79	26.00	0.05	4.827	6.89	0.10
6.80	30.00	0.05	4.895	6.42	-0.38
6.82	12.00	0.05	3.825	6.69	-0.12
6.83	6.00	0.05	3.582	6.83	0.00
6.87	2.00	0.05	3.329	6.69	-0.18

$$\text{Oxygen (ml/l)} = \text{Soc} * (\text{V} + \text{Voffset}) * (1.0 + \text{A} * \text{T} + \text{B} * \text{T}^2 + \text{C} * \text{T}^3) * \text{OxSol}(\text{T}, \text{S}) * \exp(\text{E} * \text{P} / \text{K})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU], K = temperature [Kelvin]

OxSol(T,S) = oxygen saturation [ml/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

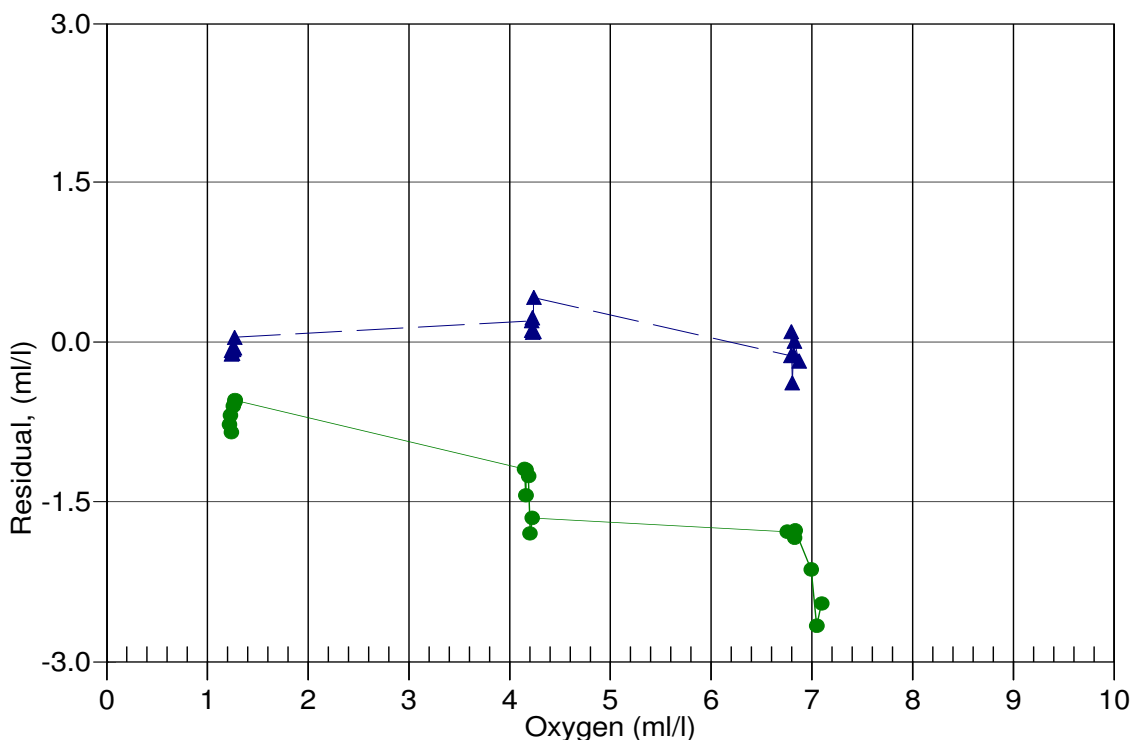

● 27-Jun-11 1.4580
 ▲ 07-Sep-12 1.0000