

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 3073
CALIBRATION DATE: 07-Jul-12

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -1.04724848e+001
h = 1.25203132e+000
i = 2.11444965e-004
j = 4.89712178e-005
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 1.66036529e-004
b = 1.25213499e+000
c = -1.04723899e+001
d = -8.34596613e-005
m = 3.6
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.89095	0.00000	0.00000
-0.9999	34.9530	2.81457	5.54781	2.81454	-0.00003
1.0001	34.9529	2.98653	5.66983	2.98656	0.00003
15.0001	34.9547	4.28680	6.51823	4.28678	-0.00002
18.5001	34.9542	4.63469	6.72702	4.63473	0.00003
29.0001	34.9503	5.72180	7.34085	5.72176	-0.00004
32.5001	34.9372	6.09469	7.53985	6.09472	0.00003


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

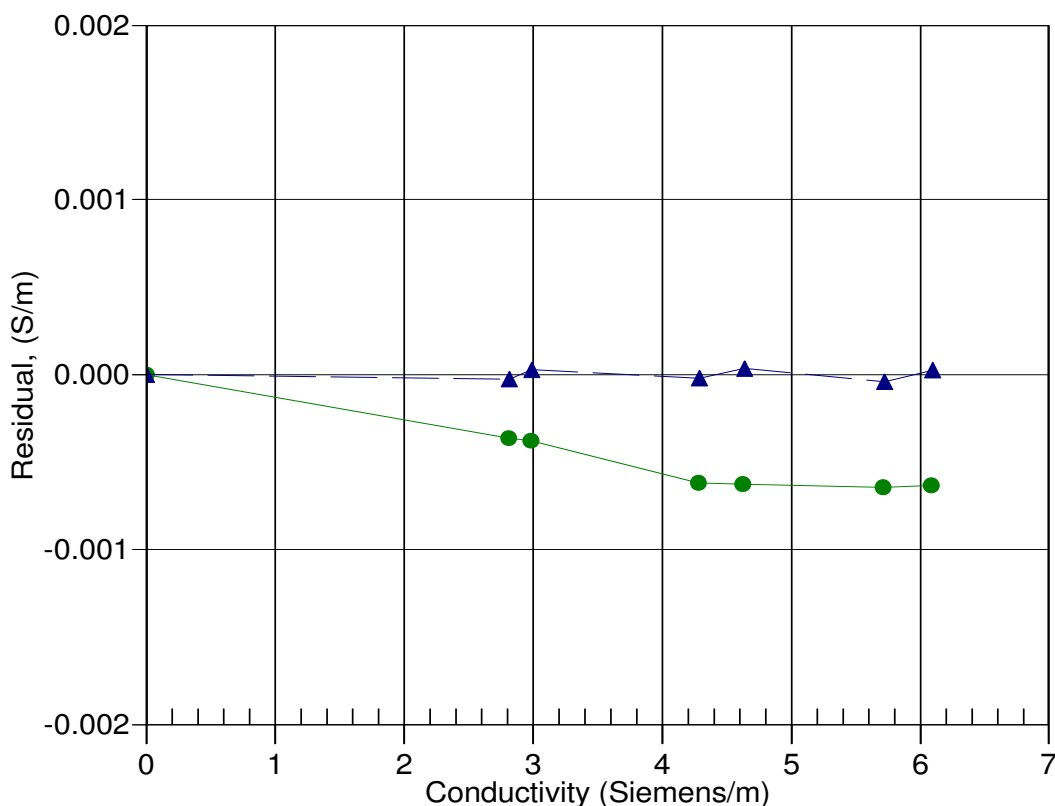

● 15-Dec-10 1.0001209
▲ 07-Jul-12 1.0000000