

SBE 41CP CERTIFICATES

CTD Serial Number 41CP-4271

Instrument Configuration.....	1
DC - Coefficient Output File.....	2
Temperature Calibration Sheet.....	3
Conductivity Calibration Sheet.....	4
Pressure Calibration Sheet.....	5

SEA-BIRD ELECTRONICS, INC.
1808 136th Place NE
Bellevue, Washington 98005 USA
Phone: (425) 643 9866
Fax: (425) 643 9954
Email: seabird@seabird.com

SBE 41CP Instrument Configuration

Model Number: SBE 41CP

Serial Number: 41CP-4271

Part Number: 90365.060

Description : APEX SBE 41CP Configuration

Firmware Version: 2.0

Pressure Type: Druck

Pressure Range: 2000 Dbar

Pressure Serial Number: 3469212

SBE 41CP UW V 2.0 SERIAL NO. 4271

temperature: 17-jan-12

TA0 = 5.405192e-05

TA1 = 2.747246e-04

TA2 = -2.470325e-06

TA3 = 1.526556e-07

conductivity: 17-jan-12

G = -9.853241e-01

H = 1.483031e-01

I = -4.217637e-04

J = 5.257568e-05

CPCOR = -9.570001e-08

CTCOR = 3.250000e-06

WBOTC = -3.869476e-08

pressure S/N = 3469212, range = 2900 psia: 10-jan-12

PA0 = 2.171991e-01

PA1 = 1.405472e-01

PA2 = -3.709155e-08

PTCA0 = 4.406584e+01

PTCA1 = 1.253901e-01

PTCA2 = -2.472732e-03

PTCB0 = 2.518463e+01

PTCB1 = 3.250000e-04

PTCB2 = 0.000000e+00

PTHA0 = -6.874124e+01

PTHA1 = 5.199935e-02

PTHA2 = -5.965373e-07

POFFSET = 0.000000e+00

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 4271
CALIBRATION DATE: 17-Jan-12

SBE 41cp TEMPERATURE CALIBRATION DATA
ITS-90 TEMPERATURE SCALE


ITS-90 COEFFICIENTS

a0 = 5.405192e-005
a1 = 2.747246e-004
a2 = -2.470325e-006
a3 = 1.526556e-007

BATH TEMP (ITS-90)	INSTRUMENT OUTPUT	INST TEMP (ITS-90)	RESIDUAL (ITS-90)
1.0000	634488.3	1.0001	0.0001
4.5000	541428.7	4.4999	-0.0001
15.0000	343110.5	15.0001	0.0001
18.5000	296564.8	18.5000	0.0000
23.9940	237318.2	23.9939	-0.0001
29.0000	194892.6	29.0000	0.0000
32.5000	170390.4	32.5000	0.0000

Temperature ITS-90 = $1/\{a_0 + a_1[\ln(n)] + a_2[\ln^2(n)] + a_3[\ln^3(n)]\} - 273.15$ (°C)

Residual = instrument temperature - bath temperature

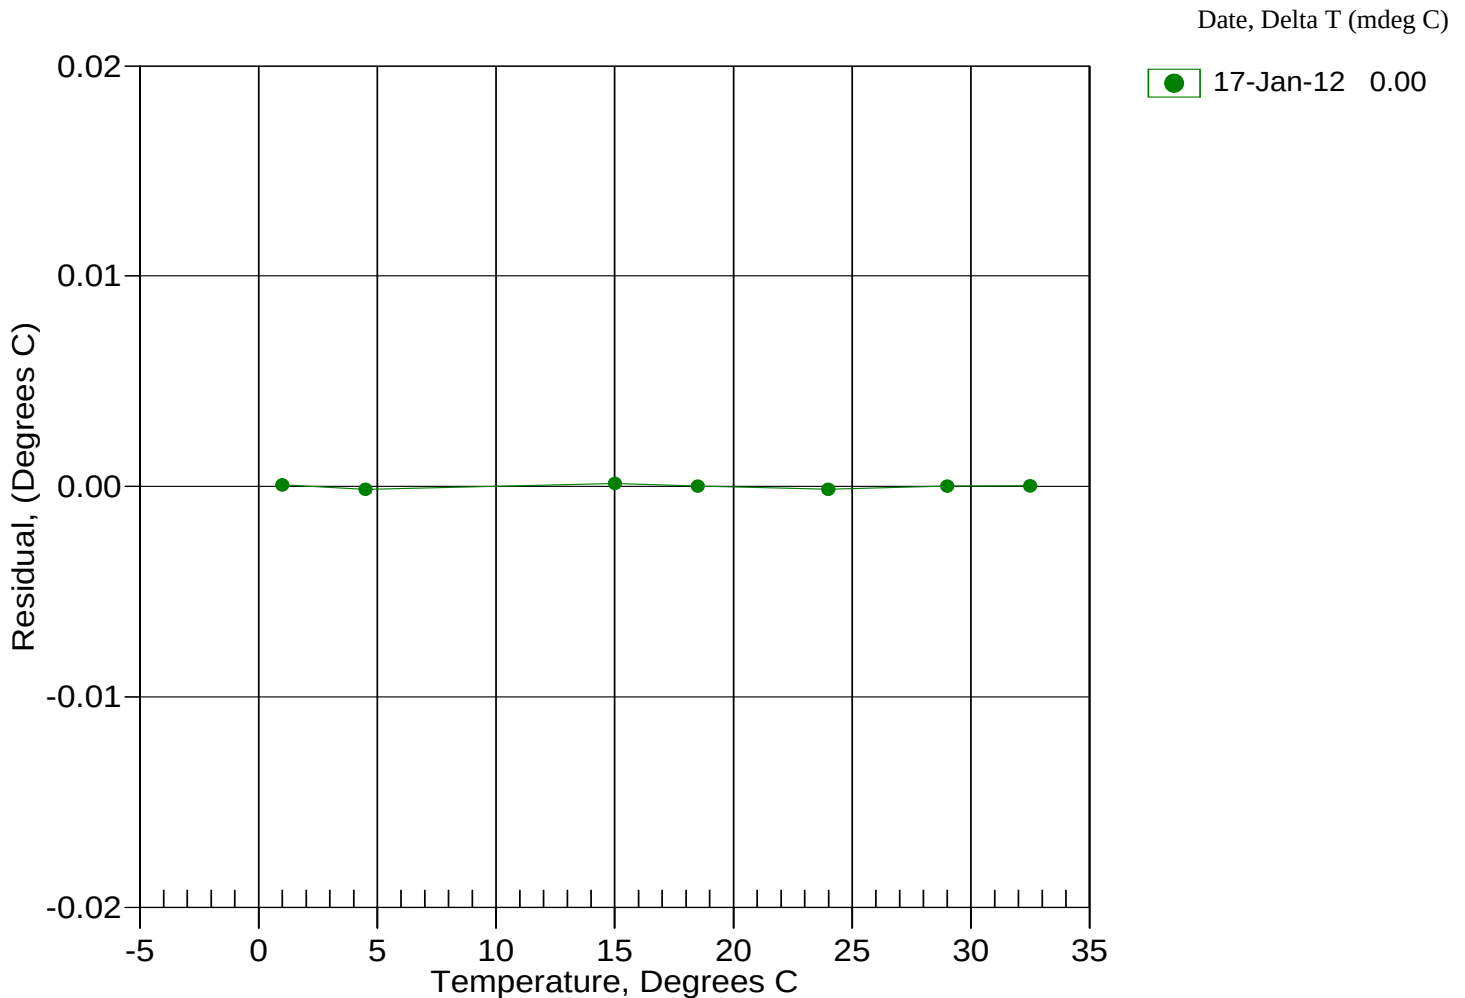

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 4271
CALIBRATION DATE: 17-Jan-12

SBE 41cp CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -9.853241e-001
h = 1.483031e-001
i = -4.217637e-004
j = 5.257568e-005

CPcor = -9.5700e-008
CTcor = 3.2500e-006
WBOTC = -3.8695e-008


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (Hz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
22.0000	0.0000	0.00000	2584.04	0.00000	0.00000
1.0000	34.8824	2.98108	5185.13	2.98108	0.00001
4.5000	34.8623	3.28864	5381.94	3.28863	-0.00001
15.0000	34.8192	4.27193	5967.04	4.27192	-0.00001
18.5000	34.8101	4.61764	6159.27	4.61763	-0.00000
23.9940	34.8002	5.17588	6457.31	5.17589	0.00001
29.0000	34.7946	5.69916	6724.34	5.69916	-0.00000
32.5000	34.7908	6.07205	6908.11	6.07204	-0.00000

$f = \text{INST FREQ} * \sqrt{1.0 + \text{WBOTC} * t} / 1000.0$

Conductivity = $(g + hf^2 + if^3 + jf^4) / (1 + \delta t + \epsilon p)$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; $\delta = \text{CTcor}$; $\epsilon = \text{CPcor}$;

Residual = instrument conductivity - bath conductivity

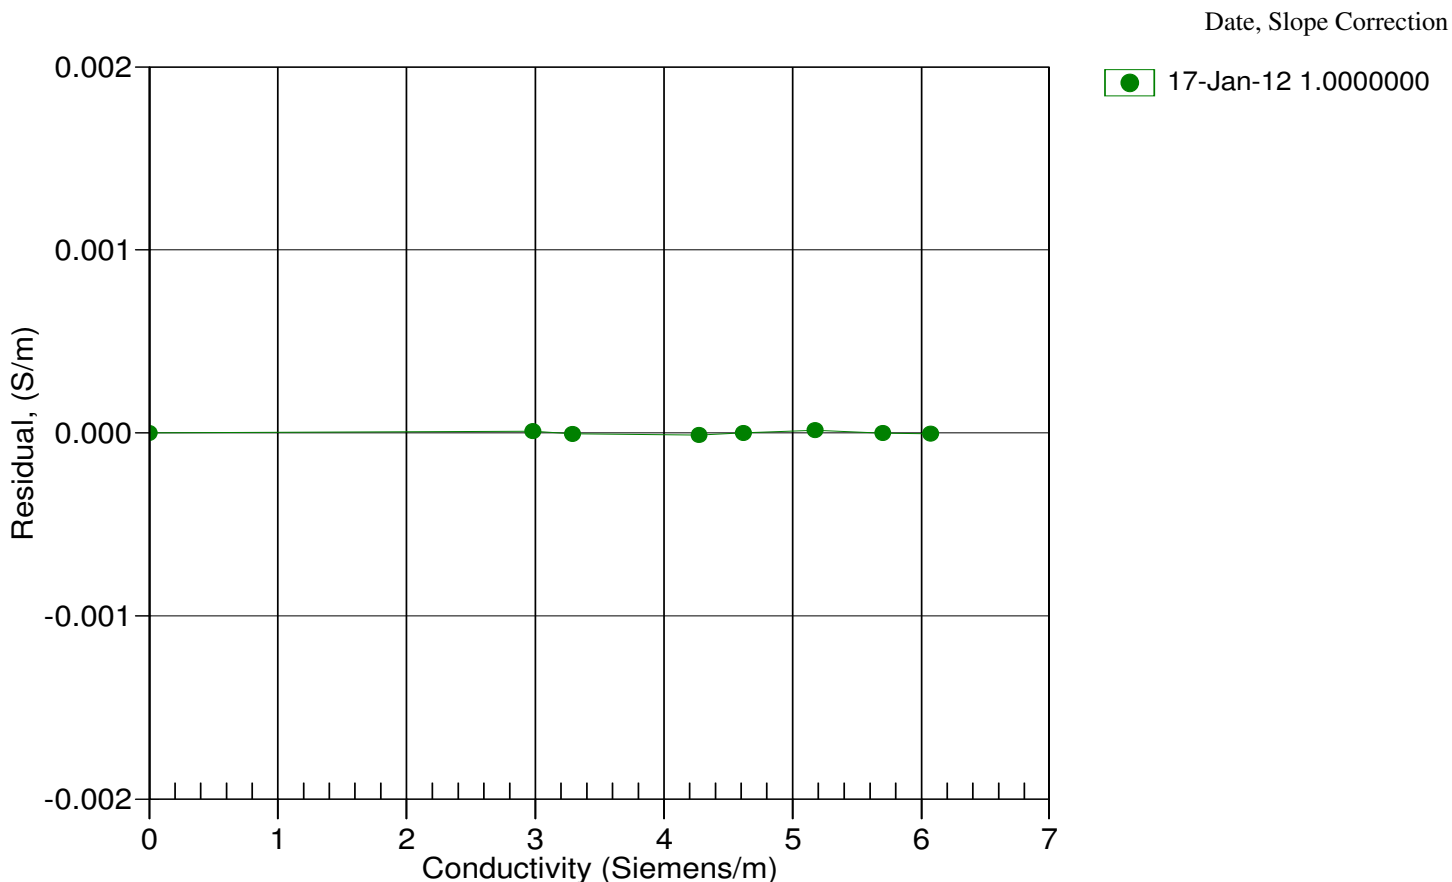

Sea-Bird Electronics, Inc.

13431 NE 20th Street, Bellevue, WA 98005-2010 USA

Phone: (+1) 425-643-9866 Fax (+1) 425-643-9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 4271

CALIBRATION DATE: 10-Jan-12

SBE 41cp PRESSURE CALIBRATION DATA

2900 psia S/N 3469212

COEFFICIENTS:

PA0 = 2.171991e-001

PA1 = 1.405472e-001

PA2 = -3.709155e-008

PTHA0 = -6.874124e+001

PTHA1 = 5.199935e-002

PTHA2 = -5.965372e-007

PTCA0 = 4.406584e+001

PTCA1 = 1.253901e-001

PTCA2 = -2.472732e-003

PTCB0 = 2.518463e+001

PTCB1 = 3.250000e-004

PTCB2 = 0.000000e+000

PRESSURE SPAN CALIBRATION

PRESSURE PSIA	INST OUTPUT	THERMISTOR OUTPUT	COMPUTED PRESSURE	ERROR %FSR
14.81	149.0	1764.3	14.74	-0.00
591.75	4261.8	1764.6	591.97	0.01
1169.23	8385.1	1764.6	1169.41	0.01
1746.76	12516.9	1765.3	1746.78	0.00
2324.19	16658.2	1765.8	2324.20	0.00
2901.47	20808.2	1766.2	2901.56	0.00
2324.27	16658.0	1765.2	2324.17	-0.00
1746.97	12517.1	1764.7	1746.81	-0.01
1169.40	8384.1	1764.2	1169.27	-0.00
591.63	4259.6	1762.8	591.66	0.00
14.81	148.9	1762.4	14.73	-0.00

THERMAL CORRECTION

TEMP ITS90	PRESS TEMP	INST OUTPUT
32.50	1992.50	151.87
29.00	1922.00	152.22
23.99	1821.70	152.35
18.50	1710.90	152.11
15.00	1641.60	151.64
4.50	1432.00	151.02
1.00	1362.50	150.78

TEMP (ITS90)	SPAN (mV)
-5.00	25.18
35.00	25.20

$$y = \text{thermistor output}; t = \text{PTHA0} + \text{PTHA1} * y + \text{PTHA2} * y^2$$

$$x = \text{pressure output} - \text{PTCA0} - \text{PTCA1} * t - \text{PTCA2} * t^2$$

$$n = x * \text{PTCB0} / (\text{PTCB0} + \text{PTCB1} * t + \text{PTCB2} * t^2)$$

$$\text{pressure (psia)} = \text{PA0} + \text{PA1} * n + \text{PA2} * n^2$$

Date, Avg Delta P %FS

10-Jan-12 0.00

