


PO Box 518  
620 Applegate St.  
Philomath, OR 97370

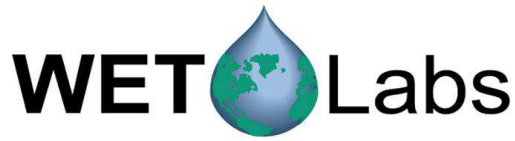

(541) 929-5650  
Fax (541) 929-5277  
[www.wetlabs.com](http://www.wetlabs.com)

## ac-s Calibration

Date	7/16/2015	Customer	U of Maine - Jim Loftin	RO #	026614
S/N #	ACS007	Technician	Cad/JGM	Cal #	14

---

Wavelength range:	400 to 730 nm	
Tcal:	22.5 deg C	
Ical:	26.5 deg C	
Acal:	29.2 deg C	
Temperature range:	8.5 to	35.0 deg C
Zero:	25.5 deg C	

---

### Definitions

Wavelength range: Wavelengths for which instrument use is recommended.

Tcal: Water temperature in flow tubes during water calibration.

Ical: Internal instrument temperature during water calibration.

Acal: Internal instrument temperature when recording air offsets in the \*.cal file.

Temperature range: Recommended internal instrument operating range.

Zero: Internal instrument temperature at which the temperature correction is zero in the device file.