

# SBE 16plus-IM V2 SEACAT Reference Sheet

(see SBE 16plus-IM V2 User's Manual for complete details)

## Sampling Modes



- **Polled** – 16plus-IM V2 takes one sample and transmits data.
- **Autonomous** – At pre-programmed intervals, 16plus-IM V2 wakes up, samples, stores data in FLASH memory, and powers off.
- **Combo** – Last Autonomous sampling data is transmitted.

## Setup

1. Double click on SeatermV2.exe. In Instruments menu, select *SBE 16plus V2 IM*. SeatermIM opens.
2. In Communications menu, select *Configure*. In dialog box, input Comm port and baud rate. Set ID to *Automatically get ID* for 1 16plus-IM V2 on line; set ID to *Use fixed ID* for multiple IM instruments on line. Click OK.
3. SeatermIM automatically connects to 16plus-IM V2. As it connects, it sends **#iiGetHD** and displays response, and then fills Send Commands window with list of commands for your 16plus-IM V2.
4. Ensure all data has been uploaded from memory, and then send **#iiInitLogging** to make entire memory available for recording. If **#iiInitLogging** is not sent, data will be stored after last recorded sample.
5. Set Date and Time (**#iiDateTime=**).
6. Set up other parameters as desired — see *Command Instructions and List*.

## Deployment

1. Install fresh batteries:
  - A. *Remove modem end cap*: Wipe dry housing/end cap seam. Remove 3 flat Phillips-head screws from end cap. Pull end cap out. Disconnect Molex connector connecting end cap to battery pack. Wipe O-ring mating surfaces in housing with lint-free cloth.
  - B. *Remove battery cover plate and batteries*: Remove 3 Phillips-head screws and washers from battery cover plate; remove cover plate. Turn 16plus-IM V2 over and remove batteries.
  - C. *Reinstall batteries, cover plate, and end cap*: Install new batteries, with + terminals against flat battery contacts and - terminals against spring contacts. Reinstall battery cover plate and 3 screws/washers. Remove water from O-rings and mating surfaces with lint-free cloth. Inspect O-rings and mating surfaces for dirt, nicks, and cuts. Clean as necessary. Apply light coat of O-ring lubricant to O-ring and mating surfaces. Plug Molex connector together. Fit end cap into housing. Reinstall 3 Phillips-head screws to secure.
2. Attach 16plus-IM V2 to insulated mooring cable with Sea-Bird mounting brackets. Install (optional) ICC on mooring cable.
3. See 16plus-IM V2 manual for SIM wiring and configuration; see IMM manual for IMM wiring and configuration.

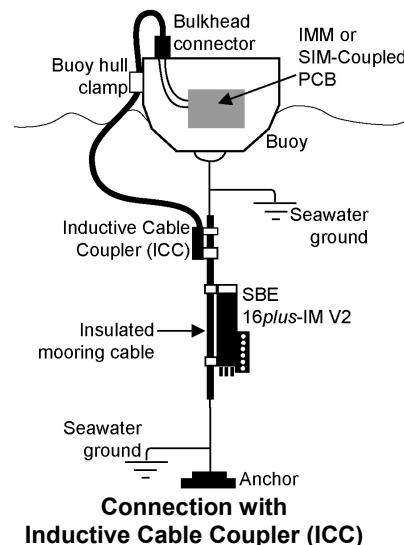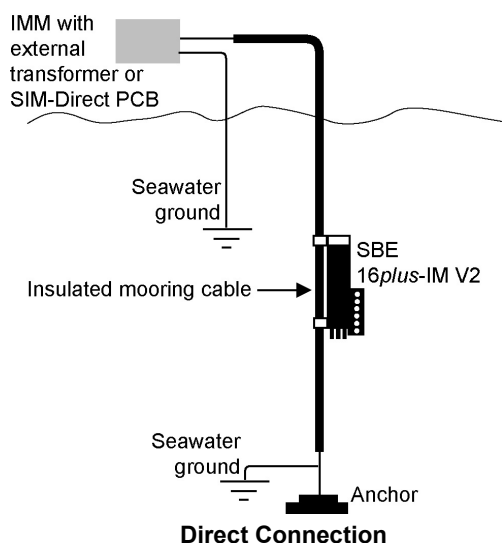

## Data Upload (see manual for fast upload via internal RS-232 connector)

1. Double click on SeatermV2.exe. In Instruments menu, select *SBE 16plus V2 IM*. SeatermIM opens.
2. In Communications menu, select *Configure*. In dialog box, input Comm port and baud rate. Set ID to *Automatically get ID* for 1 16plus-IM V2 on line; set ID to *Use fixed ID* for multiple IM instruments on line. Click OK.
3. SeatermIM automatically connects to 16plus-IM V2. As it connects, it sends **#iiGetHD** and displays response, and then fills Send Commands window with list of commands for your 16plus-IM V2.
4. If sampling autonomously (logging), command 16plus-IM V2 to stop logging by sending **#iiStop**.
5. Click Upload menu to upload stored data.
6. Run SBE Data Processing to convert uploaded .hex file to .cnv file for use by other modules in data processing software. Process file and review data to ensure all data has been uploaded.

## Command Instructions and List

Shown below are the commands used most commonly in the field. See the Manual for complete listing and detailed descriptions.

Function	Category	Command	Description	
IMM Commands	-		See the IMM manual.	
SIM Commands	Power-On	<b>PwrOn</b>	Send wakeup tone to <b>all 16plus-IM V2s</b> .	
		<b>PwrOff</b>	Send power off command to <b>all 16plus-IM V2s</b> . Logging and memory unaffected.	
		<b>AutoPwrOn=x</b>	<b>x=Y</b> (default): Send <b>PwrOn</b> to <b>16plus-IM V2s</b> when power applied to SIM. <b>x=N</b> : Do not.	
	Status	<b>DS</b>	Display SIM firmware version and setup parameters.	
	Comms	<b>Baud=x</b>	<b>x=</b> baud from SIM to computer (1200, 2400, 4800, or 9600). Default 9600.	
		<b>DataNNMax=x</b>	<b>x=</b> timeout that applies to <b>iiData</b> or <b>Dataii</b> ; default 1000 milliseconds.	
<b>RelayMax=x</b>		<b>x=</b> timeout that applies to all other commands; default 20 seconds.		
<b>EchoOn EchoOff</b>		Echo characters received from computer. Do not.		
16plus-IM V2 Communication Microcontroller Commands	Global	<b>DateTime=mmddyyyhhmmss</b>	Set <b>all</b> real-time clocks: month, day, year, hour, minute, second.	
		<b>GData</b>	Command <b>all 16plus-IM V2</b> communication microcontrollers to get data from <b>16plus-IM V2</b> acquisition microcontrollers. Communication microcontrollers hold data in buffer until receiving <b>iiData</b> or <b>Dataii</b> .	
	Get Data	<b>iiData</b> or <b>Dataii</b>	Get data obtained with <b>GData</b> from <b>16plus-IM V2</b> with ID= <b>ii</b> .	
	16plus-IM V2 ID	<b>ID?</b>	Display <b>16plus-IM V2</b> ID (ID = <b>ii</b> , where <b>ii=0</b> to 99)	
		<b>*ID=ii</b>	Set ID to <b>ii</b> ( <b>ii=0</b> to 99). Only one <b>16plus-IM V2</b> can be on line or all <b>16plus-IM V2s</b> on line will have same ID. Computer responds by requesting verification.	
	Status	<b>!iiDS</b>	Display communication microcontroller status.	
	Timeout	<b>!iiWait=x</b>	<b>x=</b> time for communication microcontroller to wait for response from acquisition microcontroller. Range 2 – 600 seconds.	
16plus-IM V2 Acquisition Microcontroller Commands (ii = 16plus-IM V2 ID)	Status	<b>#iiGetCD</b>	Get and display configuration data (setup parameters).	
		<b>#iiGetSD</b>	Get and display status data.	
		<b>#iiGetCC</b>	Get and display calibration coefficients.	
		<b>#iiGetEC</b>	Get and display event counter data.	
		<b>#iiResetEC</b>	Reset all events in event counter.	
		<b>#iiGetHD</b>	Get and display hardware data.	
		<b>#iiDS</b>	Display status and setup parameters.	
	General Setup	<b>#iiDCal</b>	Display calibration coefficients.	
		<b>#iiDateTime=mmddyyyhhmmss</b>	Set real-time clock month, day, year, hour, minute, second.	
		<b>#iiOutputExecutedTag=x</b>	<b>x=Y</b> : Display XML Executing and Executed tags. <b>x=N</b> : Do not.	
		<b>#iiPumpMode=x</b>	<b>x=0</b> : No pump. <b>x=1</b> : Run pump for 0.5 seconds before each sample. <b>x=2</b> : Run pump during each sample.	
		<b>#iiNCycles=x</b>	<b>x=</b> number of samples to take and average every <b>#iiSampleInterval</b> seconds.	
	Pressure Setup	<b>#iiInitLogging</b>	After uploading all data, send this command before starting to log to make entire memory available for recording. If not sent, data stored after last sample.	
		<b>#iiBioWiper=x</b>	<b>x=Y</b> : Configuration includes ECO-FL fluorometer with Bio-Wiper. <b>x=N</b> : Does not.	
		<b>#iiRefPress=x</b>	<b>x=</b> reference pressure (decibars) (for <b>16plus-IM V2</b> without pressure sensor).	
	Voltage Sensor Setup	<b>#iiParosIntegration=x</b>	<b>x=</b> integration time (sec) for Quartz pressure sensor (1 – 600 sec; default 1 sec).	
		<b>#iiVolt0=x, #iiVolt1=x, #iiVolt2=x, #iiVolt3=x, #iiVolt4=x, #iiVolt5=x</b>	<b>x=Y</b> : Enable external voltage (voltage 0, 1, 2, 3, 4, or 5). <b>x=N</b> : Do not.	
	RS-232 Setup	<b>#iiDelayBeforeSampling=x</b>	<b>x=</b> time (sec) to wait after powering external voltages and RS-232 sensors before sampling (0-600 sec).	
		<b>#iiSBE38=x</b>	<b>x=Y</b> : Enable SBE 38 secondary temperature sensor. <b>x=N</b> : Do not.	
		<b>#iiSBE50=x</b>	<b>x=Y</b> : Enable SBE 50 secondary pressure sensor. <b>x=N</b> : Do not.	
		<b>#iiWetLabs=x</b>	<b>x=Y</b> : Enable WET Labs RS-232 sensor. <b>x=N</b> : Do not.	
		<b>#iiGTD=x</b>	<b>x=Y</b> : Enable GTD. <b>x=N</b> : Do not.	
		<b>#iiDualGTD=x</b>	<b>x=Y</b> : Enable dual GTDs. <b>x=N</b> : Do not.	
	Output Format Setup	<b>#iiOptode=x</b>	<b>x=Y</b> : Enable Aanderaa Optode. <b>x=N</b> : Do not.	
		<b>#iiOutputFormat=x</b>	<b>x=0</b> : output raw data, Hex. <b>x=1</b> : converted data, Hex. <b>x=2</b> : raw data, decimal. <b>x=3</b> : converted data, decimal. <b>x=5</b> : converted data, decimal, XML.	
		<b>#iiOutputSal=x</b>	<b>x=Y</b> : Calculate salinity (psu) (if <b>#iiOutputFormat=3</b> or <b>5</b> ). <b>x=N</b> : Do not.	
		<b>#iiOutputSV=x</b>	<b>x=Y</b> : Calculate sound velocity (m/sec) (if <b>#iiOutputFormat=3</b> or <b>5</b> ). <b>x=N</b> : Do not.	
		<b>#iiOutputUCSD=x</b>	<b>x=Y</b> : Calculate sigma-t, battery voltage, operating current (if <b>#iiOutputFormat=3</b> or <b>5</b> ). <b>x=N</b> : Do not.	
	Autonomous Sampling (Logging)	<b>#iiOutputSampleNumber=x</b>	<b>x=Y</b> : Output sample number with data (if <b>#iiOutputFormat=3</b> or <b>5</b> ). <b>x=N</b> : Do not.	
		<b>#iiSampleInterval=x</b>	<b>x=</b> interval between samples (10 - 14400 seconds).	
		<b>#iiStartNow</b>	Start logging now. Data stored in FLASH memory.	
		<b>#iiStartDateTime=mmddyyyhhmmss</b>	Delayed logging start: month day year, hour, minute, second.	
		<b>#iiStartLater</b>	Start logging at delayed start date and time. Data stored in FLASH memory.	
		<b>#iiStop</b>	Stop logging or waiting to log. Must send this command before uploading data.	
	Polled Sampling	<b>#iiSL</b>	Output last sample from buffer.	
		<b>#iiSLT</b>	Output last sample from buffer, take new sample, and store in buffer.	
		<b>#iiTS</b>	Take sample, store data in buffer, and output data.	
		<b>#iiTSS</b>	Take sample, <b>store in buffer and FLASH memory</b> , and output data.	
	Data Upload	<b>GetLastSamples:x</b>	Output last <b>x</b> samples from FLASH memory.	
		<b>GetSamples:b,e</b> or <b>#iiDDb,e</b>	Upload data from scan <b>b</b> to <b>e</b> . Send <b>#iiStop</b> before sending this.	
			<b>GetHeaders:b,e</b> or <b>#iiDHb,e</b>	Upload headers from header <b>b</b> to <b>e</b> .